

Air Quality



Website: www.acuityhk.com
 Unit E, 12/F, Ford Glory Plaza
 Nos. 37-39 Wing Hong Street,
 Cheung Sha Wan, Kowloon
 Tel: (852) 2698 6833
 Fax: (852) 2698 9383

Sibata LD-5R K-Factor Verification Test by Total Suspended Particulates HVS Test Report

Verification Test Date: 3-Dec-22 to 4-Dec-22
 Next Verification Test Date: 2-Dec-23
 Unit-under-Test- Model No. Sibata LD-5R
 Unit-under-Test Serial No. OZ4545
 Our Report Reference No. RPT-22-HVS-0026
 Calibration Location: AM2, Located near the Leachate Treatment Works within the NENT Landfill

Standard Equipment Information			
Verification Equipment Type	Tisch TSP HVS	Tisch HVS Calibrator	
Standard Equipment Model No.	TE-5170X	TE-5025A	
Equipment serial no.	MFC 1106	3465	
Last Calibration Date	1-Dec-22	28-Jun-22	
Next Calibration Date	31-Jan-23	27-Jun-23	

Verification Test No.	Date	Time			K-Factor	Counts/Minute (R)	Total Counts (TC)	TSP Sample ID No.	Dust Concentration (ug/m3), (C)	
		Start-time	End-time	Elapsed Time (in min)					K-Factor (K=C/R)	x-axis
1	3/12/2022	194.73	198.08	201.00	0.00120	51	10251	R222043/1	61	
2	3/12/2022	198.08	201.27	191.40	0.00102	34	6444	R222043/2	34	
3	3/12/2022	201.27	204.35	184.80	0.00111	44	8193	R222043/3	49	
4	4/12/2022	252.37	255.36	179.40	0.00122	55	9927	R222044/1	67	
5	4/12/2022	255.38	258.38	180.00	0.00120	52	9360	R222044/2	62	
6	4/12/2022	258.38	261.38	180.00	0.00112	63	11340	R222044/3	70	
					0.00114					

K-Factor to be inputted in LD-5R (corrected 1 decimal point): 1.1

By Linear Regression of y on x:


slope, mh= 1.3204

intercept, ch= -8.3520

*Correlation Coefficient, R= 0.9780

Verification Test Result: Strong Correlation, Results were accepted.

* If the Correlation Coefficient, R is <0.5. Checking and Re-verification are required.

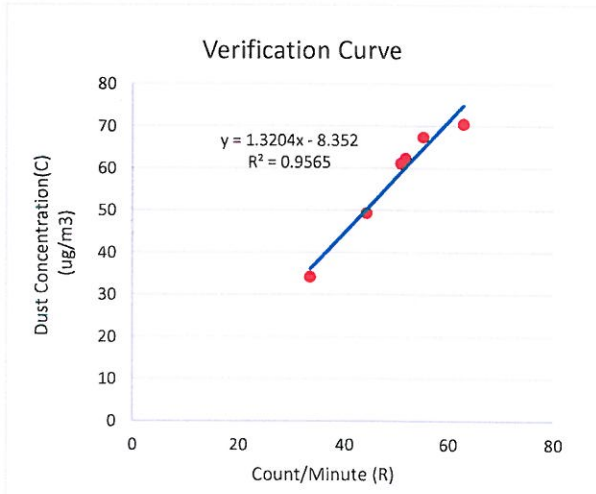

Verified By: [Signature]
 Technical Manager

Date: 05-12-2022

Sibata LD-5R K-Factor Verification Test by Total Suspended Particulates HVS Test Report

Verification Test Date: 3-Dec-22 to 4-Dec-22
 Next Verification Test Date: 2-Dec-23
 Unit-under-Test- Model No.: Sibata LD-5R
 Unit-under-Test Serial No.: 882106
 Our Report Reference No.: RPT-22-HVS-0027
 Calibration Location: AM2, Located near the Leachate Treatment Works within the NENT Landfill

Standard Equipment Information			
Verification Equipment Type	Tisch TSP HVS	Tisch HVS Calibrator	
Standard Equipment Model No.	TE-5170X	TE-5025A	
Equipment serial no.	MFC 1106	3465	
Last Calibration Date	1-Dec-22	28-Jun-22	
Next Calibration Date	31-Jan-23	27-Jun-23	

Verification Test No.	Date	Time			K-Factor K-Factor (K=C/R)	Counts/ Minute (R)	Total Counts (TC)	TSP Sample ID No.	Dust Concentration (ug/m3), (C)
		Start-time	End-time	Elapsed Time (in min)					y axis
1	3/12/2022	194.73	198.08	201.00	0.00123	50	9983	R222043/1	61
2	3/12/2022	198.08	201.27	191.40	0.00092	37	7146	R222043/2	34
3	3/12/2022	201.27	204.35	184.80	0.00103	48	8870	R222043/3	49
4	4/12/2022	252.37	255.36	179.40	0.00108	62	11183	R222044/1	67
5	4/12/2022	255.38	258.38	180.00	0.00110	57	10260	R222044/2	62
6	4/12/2022	258.38	261.38	180.00	0.00108	65	11760	R222044/3	70
					0.00107				

K-Factor to be inputted in LD-5R (corrected 1 decimal point): 1.1

By Linear Regression of y on x:


slope, mh= 1.2417

intercept, ch= -8.6314

*Correlation Coefficient, R= 0.9513

Verification Test Result: Strong Correlation, Results were accepted.

* If the Correlation Coefficient, R is <0.5. Checking and Re-verification are required.

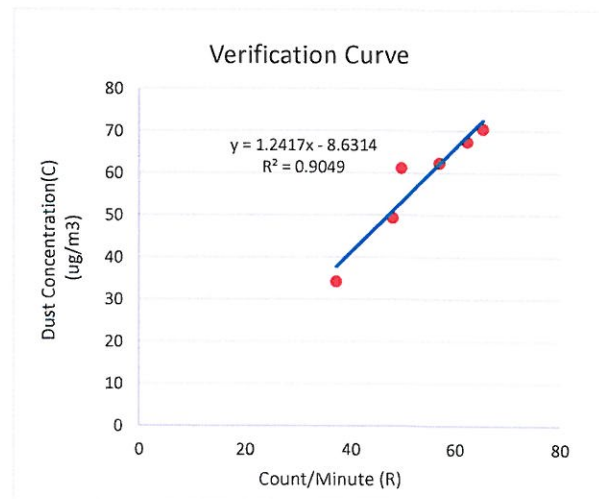

Verified By: IA
 Technical Manager

Date: 05-12-2022

Sibata LD-5R K-Factor Verification Test by Total Suspended Particulates HVS Test Report

Verification Test Date: 3-Dec-22 to 4-Dec-22
 Next Verification Test Date: 2-Dec-23
 Unit-under-Test- Model No. Sibata LD-5R
 Unit-under-Test Serial No. 882110
 Our Report Reference No. RPT-22-HVS-0025
 Calibration Location: AM2, Located near the Leachate Treatment Works within the NENT Landfill

Standard Equipment Information			
Verification Equipment Type	Tisch TSP HVS	Tisch HVS Calibrator	
Standard Equipment Model No.	TE-5170X	TE-5025A	
Equipment serial no.	MFC 1106	3465	
Last Calibration Date	1-Dec-22	28-Jun-22	
Next Calibration Date	31-Jan-23	27-Jun-23	

Verification Test No.	Date	Time			K-Factor	Counts/Minute (R)	Total Counts (TC)	TSP Sample ID No.	Dust Concentration (ug/m3), (C)	
		Start-time	End-time	Elapsed Time (in min)					K-Factor (K=C/R)	x-axis
1	3/12/2022	194.73	198.08	201.00	0.00101	61	12194	R222043/1	61	
2	3/12/2022	198.08	201.27	191.40	0.00089	38	7337	R222043/2	34	
3	3/12/2022	201.27	204.35	184.80	0.00108	46	8439	R222043/3	49	
4	4/12/2022	252.37	255.36	179.40	0.00110	61	11003	R222044/1	67	
5	4/12/2022	255.38	258.38	180.00	0.00112	56	10080	R222044/2	62	
6	4/12/2022	258.38	261.38	180.00	0.00104	68	12180	R222044/3	70	
					0.00104					

K-Factor to be inputted in LD-5R (corrected 1 decimal point): 1.0

By Linear Regression of y on x:

slope, mh= 1.1984

intercept, ch= -8.3267


*Correlation Coefficient, R= 0.9700

Verification Test Result: Strong Correlation, Results were accepted.

* If the Correlation Coefficient, R is <0.5. Checking and Re-verification are required.

Verified By: 
 Technical Manager

Date: 05-12-2022

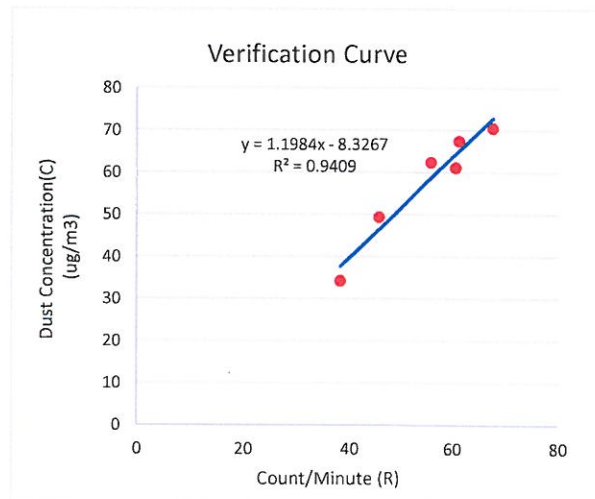

Sibata LD-5R K-Factor Verification Test by Total Suspended Particulates HVS Test Report

Verification Test Date: 3-Dec-22 to 4-Dec-22
 Next Verification Test Date: 2-Dec-23
 Unit-under-Test- Model No. Sibata LD-5R
 Unit-under-Test Serial No. 942532
 Our Report Reference No. RPT-22-HVS-0024
 Calibration Location: AM2, Located near the Leachate Treatment Works within the NENT Landfill

Standard Equipment Information			
Verification Equipment Type	Tisch TSP HVS	Tisch HVS Calibrator	
Standard Equipment Model No.	TE-5170X	TE-5025A	
Equipment serial no.	MFC 1106	3465	
Last Calibration Date	1-Dec-22	28-Jun-22	
Next Calibration Date	31-Jan-23	27-Jun-23	

Verification Test No.	Date	Time			K-Factor K-Factor (K=C/R)	Counts/ Minute (R) x-axis	Total Counts (TC)	TSP Sample ID No.	Dust Concentration (ug/m3), (C) y axis
		Start-time	End-time	Elapsed Time (in min)					
1	3/12/2022	194.73	198.08	201.00	0.00111	55	11122	R222043/1 61	
2	3/12/2022	198.08	201.27	191.40	0.00093	37	7082	R222043/2 34	
3	3/12/2022	201.27	204.35	184.80	0.00110	45	8316	R222043/3 49	
4	4/12/2022	252.37	255.36	179.40	0.00113	60	10704	R222044/1 67	
5	4/12/2022	255.38	258.38	180.00	0.00120	52	9360	R222044/2 62	
6	4/12/2022	258.38	261.38	180.00	0.00104	68	12180	R222044/3 70	

0.00108

K-Factor to be inputted in LD-5R (corrected 1 decimal point): 1.1

By Linear Regression of y on x:


slope, mh= 1.1919

intercept, ch= -5.3851

*Correlation Coefficient, R= 0.9543

Verification Test Result: Strong Correlation, Results were accepted.

* If the Correlation Coefficient, R is <0.5. Checking and Re-verification are required.

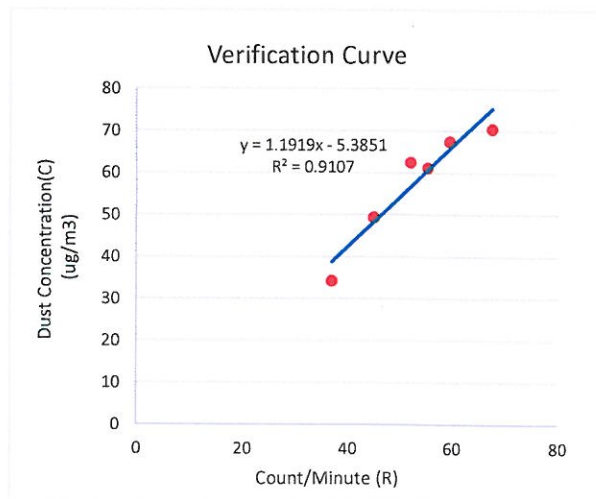

Verified By: [Signature]
Technical Manager

Date: 05-12-2022

HIVOL SAMPLER CALIBRATION DATA SHEET (TSP)

Site Information

Location:	NENTX	Site ID:	AM1	Date:	30-Jan-2023
Serial No:	1105	Model:	TE-5170X	Operator:	Andy Li

Ambient Condition

Actual Pressure during Calibration (P_a) (mm Hg):	765.1	Actual Temperature during Calibration (T_a) (deg K):	291.4
---	-------	--	-------

Calibration Orifice

Model:	TE-5025A	Slope (m_c):	2.05924
Serial No.:	3465	Intercept (b_c):	-0.01929
Calibration Due Date:	28-Jun-23	Corr. Coeff:	0.99998

Calibration Data

Plate or Test #	ΔH_2O (in)	Qa, X-Axis (m^3/min)	I, CFM (chart)	IC, Y-Axis (corrected)
1	2.20	0.740	43.0	43.63
2	3.40	0.918	47.0	47.69
3	4.60	1.066	52.0	52.76
4	5.20	1.133	54.0	54.79
5	6.00	1.216	56.0	56.82

Sampler Calibration Relationship (Qa on x-axis, IC on y-axis)

$$m = \frac{28.5644}{\text{Sampler Set Point Flow Rate (SFR) = 1.1013}} \quad b = \frac{22.1538}{\text{Sampler Chart Set Point (SSP) = 54}} \quad \text{Corr. Coeff} = 0.9971$$

Calculations

$$Q_a = 1/m_c * [\text{Sqrt}(\Delta H_2O * (P_a/P_{std})) * (T_{std}/T_a)] - b_c$$


$$IC = I * (\text{Sqrt}(P_a/P_{std}) * (T_{std}/T_a))$$

$$\text{SFR} = 1.13 (P_{std} / P_a) (T_a / T_{std})$$

$$\text{SSP} = (m * \text{SFR} + b) (\text{Sqrt}(P_a / P_{std}) (T_{std} / T_a))$$

Q_a = actual flow rate
 IC = corrected chart response
 I = actual chart response
 m_c = calibrator slope
 b_c = calibrator intercept
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)

m = sampler slope
 b = sampler intercept
 T_{std} = 298 deg K
 P_{std} = 760 mm Hg
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)
 Where 1.13 is the designed sampling flow rate of PM10 samplers, m^3/min

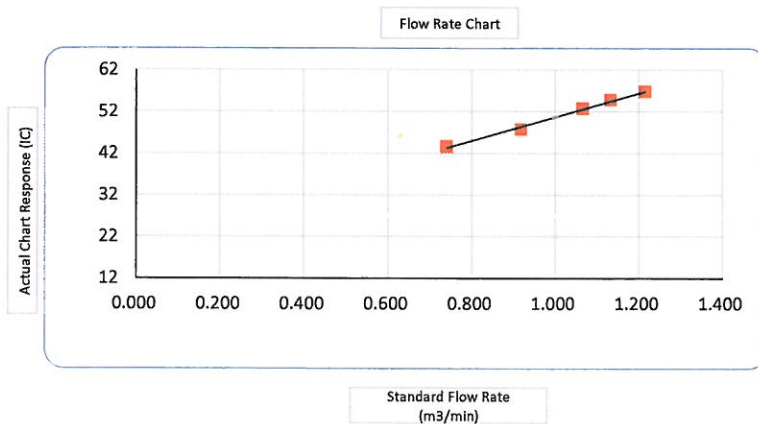

Checked by: _____



Date: _____ 30-Jan-2023

HIVOL SAMPLER CALIBRATION DATA SHEET (TSP)

Site Information

Location:	NENTX	Site ID:	AM2	Date:	30-Jan-2023
Serial No.:	1106	Model:	TE-5170X	Operator:	Andy Li

Ambient Condition

Actual Pressure during Calibration (P_a) (mm Hg):	765.1	Actual Temperature during Calibration (T_a) (deg K):	295.4
---	-------	--	-------

Calibration Orifice

Model:	TE-5025A	Slope (m_c):	2.05924
Serial No.:	3465	Intercept (b_c):	-0.01929
Calibration Due Date:	28-Jun-23	Corr. Coeff:	0.99998

Calibration Data

Plate or Test #	ΔH_2O (in)	Qa, X-Axis (m ³ /min)	I, CFM (chart)	IC, Y-Axis (corrected)
1	2.00	0.701	42.0	42.33
2	2.60	0.798	45.0	45.35
3	3.80	0.963	50.0	50.39
4	4.60	1.059	55.0	55.43
5	5.60	1.167	58.0	58.45

Sampler Calibration Relationship (Qa on x-axis, IC on y-axis)

m=	35.3651	b=	17.2173	Corr. Coeff=	0.9959
Sampler Set Point Flow Rate (SFR)=			1.1164	Sampler Chart Set Point (SSP)=	
				57	

Calculations

$$Q_a = 1/m_c * [\text{Sqrt}(\Delta H_2O * (P_a/P_{Std}) * (T_{Std}/T_a)) - b_c]$$


$$IC = I * (\text{Sqrt}(P_a/P_{Std}) * (T_{Std}/T_a))$$

$$SFR = 1.13 (P_{Std} / P_a) (T_a / T_{Std})$$

$$SSP = (m * SFR + b) (\text{Sqrt}(P_a / P_{Std}) (T_{Std} / T_a))$$

Qa = actual flow rate
 IC = corrected chart response
 I = actual chart response
 m_c = calibrator slope
 b_c = calibrator intercept
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)

m = sampler slope
 b = sampler intercept
 T_{Std} = 298 deg K
 P_{Std} = 760 mm Hg
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)
 Where 1.13 is the designed sampling flow rate of PM10 samplers, m³/min

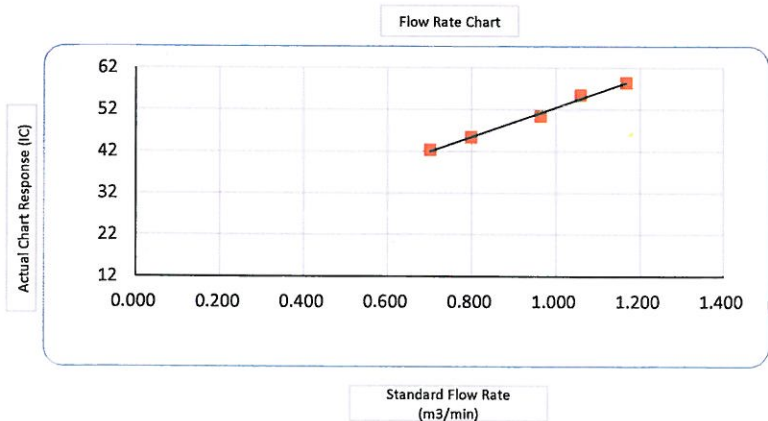

Checked by: _____ 

Date: _____ 30-Jan-2023

HIVOL SAMPLER CALIBRATION DATA SHEET (TSP)

Site Information

Location:	NENTX	Site ID:	AM3	Date:	30-Jan-2023
Serial No:	1856	Model:	TE-5170X	Operator:	Andy Li

Ambient Condition

Actual Pressure during Calibration (P_a) (mm Hg):	765.1	Actual Temperature during Calibration (T_a) (deg K):	296.9
---	-------	--	-------

Calibration Orifice

Model:	TE-5025A	Slope (m_c):	2.05924
Serial No.:	3465	Intercept (b_c):	-0.01929
Calibration Due Date:	28-Jun-23	Corr. Coeff:	0.99998

Calibration Data

Plate or Test #	ΔH_2O (in)	Qa, X-Axis (m ³ /min)	I, CFM (chart)	IC, Y-Axis (corrected)
1	1.60	0.627	44.0	44.23
2	3.00	0.855	54.0	54.28
3	4.00	0.986	57.0	57.30
4	5.00	1.101	60.0	60.31
5	6.00	1.205	64.0	64.33

Sampler Calibration Relationship (Qa on x-axis, IC on y-axis)

m=	33.5233	b=	24.0872	Corr. Coeff=	0.9921
Sampler Set Point Flow Rate (SFR)=	1.1221	Sampler Chart Set Point (SSP)=	62		

$$Q_a = 1/m_c * [\text{Sqrt}(\Delta H_2O * (P_a/P_{std}) * (T_{std}/T_a)) - b_c]$$

$$IC = I * (\text{Sqrt}(P_a/P_{std}) * (T_{std}/T_a))$$


Q_a = actual flow rate
 IC = corrected chart response
 I = actual chart response
 m_c = calibrator slope
 b_c = calibrator intercept
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)

Calculations

$$SFR = 1.13 (P_{std} / P_a) (T_a / T_{std})$$

$$SSP = (m * SFR + b) (\text{Sqrt}(P_a / P_{std}) (T_{std} / T_a))$$

m = sampler slope
 b = sampler intercept
 T_{std} = 298 deg K
 P_{std} = 760 mm Hg
 T_a = actual temperature during calibration (deg K)
 P_a = actual pressure during calibration (mm Hg)
 Where 1.13 is the designed sampling flow rate of PM10 samplers, m³/min

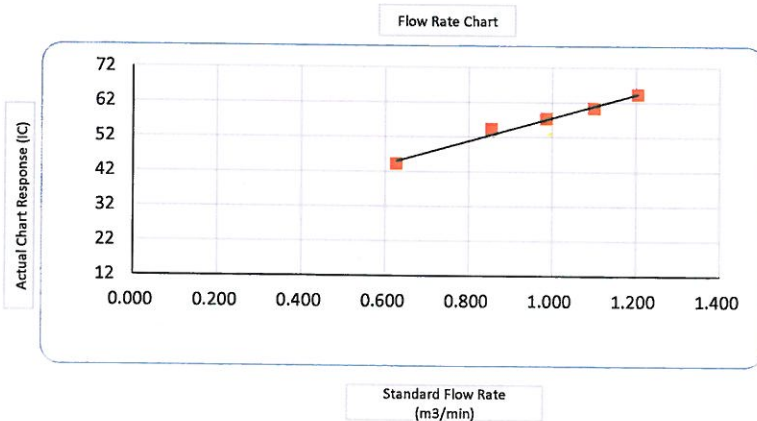

Checked by: _____

Date: _____ 30-Jan-2023

Certificate of Calibration

Calibration Certification Information			
Cal. Date: June 28, 2022	Rootsmeter S/N: 438320	Ta: 296	°K
Operator: Jim Tisch		Pa: 755.1	mm Hg
Calibration Model #: TE-5025A	Calibrator S/N: 3465		

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.4290	3.2	2.00
2	3	4	1	1.0130	6.4	4.00
3	5	6	1	0.9050	7.9	5.00
4	7	8	1	0.8590	8.8	5.50
5	9	10	1	0.7110	12.8	8.00

Data Tabulation						
Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)	
0.9961	0.6970	1.4144	0.9958	0.6968	0.8854	
0.9918	0.9791	2.0003	0.9915	0.9788	1.2522	
0.9899	1.0938	2.2364	0.9895	1.0934	1.4000	
0.9887	1.1509	2.3456	0.9883	1.1506	1.4683	
0.9834	1.3831	2.8289	0.9830	1.3826	1.7708	
QSTD	m=	2.05924	QA	m=	1.28946	
	b=	-0.01929		b=	-0.01207	
	r=	0.99998		r=	0.99998	

Calculations			
Vstd=	$\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$	Va=	$\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime
For subsequent flow rate calculations:			
Qstd=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$

Standard Conditions	
Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootsmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION
US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30

Calibration Certificate

Customer Name Paul Y Construction Co. Ltd
 Model PS200
 Serial 373075
 Tested On 16 November, 2022
 Cal Expires 16 November, 2023

Audible Alarm PASS
 Visual Alarm PASS
 Calibrated For METHANE
 100% LEL Equivalent 4.4% by VOL

Overall Results PASS



Calibration Result

Gas Applied	Range	Reading	Calibrated	Result
Zero Air	% LEL	0	0	PASS
Zero Air	% O2	20.9	20.9	PASS
Zero Air	PPM CO	0	0	PASS
Zero Air	PPM H2S	0	0	PASS

Gas Applied	Range	Reading	Calibrated	Result
50% LEL Methane	% LEL	61	50	PASS
18% VOL Oxygen	% O2	17.8	N/A	PASS
100 PPM Carbon Monoxide	PPM CO	71	100	PASS
25 PPM Hydrogen Sulphide	PPM H2S	22	25	PASS

Calibrated By Ivan Lo :



Noise

Certificate of Calibration

for

Description: Sound Level Meter
Manufacturer: NTi Audio
Type No.: XL2 (Serial No.: A2A-09696-E0)
Microphone: ACO 7052 (Serial No.:68840)
Preamplifier: NTi Audio M2211 MA220 (Serial No.:5287)

Submitted by:

Customer: Acumen Environmental Engineering and Technologies Co.
Ltd.
Address: Unit D, 12/F, Ford Glory Plaza,
Nos. 37-39 Wing Hong Street,
Cheung Sha Wan, Kowloon, Hong Kong

Upon receipt for calibration, the instrument was found to be:

- Within
 Outside

the allowable tolerance.

The test equipment used for calibration are traceable to National Standards via:

- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 24 March 2022

Date of calibration: 26 March 2022

Calibrated by: 
Calibration Technician

Certified by: 
Mr. Ng Yan Wa
Laboratory Manager

Date of issue: 26 March 2022



Certificate No.: APJ21-161-CC001

Page 1 of 4

1. Calibration Precaution:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Conditions:

Air Temperature: 22.6 °C
 Air Pressure: 1006 hPa
 Relative Humidity: 74.5 %

3. Calibration Equipment:

	Type	Serial No.	Calibration Report Number	Traceable to
Multifunction Calibrator	B&K 4226	2288467	AV200041	HOKLAS

4. Calibration Results

Sound Pressure Level

Reference Sound Pressure Level

Setting of Unit-under-test (UUT)				Applied value		UUT Reading, dB	IEC 61672 Class 1 Specification, dB
Range, dB	Freq. Weighting		Time Weighting	Level, dB	Frequency, Hz		
30-130	dBA	SPL	Fast	94	1000	94.1	±0.4

Linearity

Setting of Unit-under-test (UUT)				Applied value		UUT Reading, dB	IEC 61672 Class 1 Specification, dB
Range, dB	Freq. Weighting		Time Weighting	Level, dB	Frequency, Hz		
30-130	dBA	SPL	Fast	94	1000	94.1	Ref
				104		104.1	±0.3
				114		114.1	±0.3

Time Weighting

Setting of Unit-under-test (UUT)				Applied value		UUT Reading, dB	IEC 61672 Class 1 Specification, dB
Range, dB	Freq. Weighting		Time Weighting	Level, dB	Frequency, Hz		
30-130	dBA	SPL	Fast	94	1000	94.1	Ref
			Slow			94.1	±0.3

Certificate No.: APJ21-161-CC001



Page 2 of 4

Frequency Response

Linear Response

Setting of Unit-under-test (UUT)			Applied value		UUT Reading, dB	IEC 61672 Class 1 Specification, dB	
Range, dB	Freq. Weighting	Time Weighting	Level, dB	Frequency, Hz			
30-130	dB	SPL	Fast	94	31.5	94.0	±2.0
					63	94.1	±1.5
					125	94.1	±1.5
					250	94.0	±1.4
					500	94.1	±1.4
					1000	94.1	Ref
					2000	94.3	±1.6
					4000	94.9	±1.6
				8000	93.6	+2.1; -3.1	

A-weighting

Setting of Unit-under-test (UUT)			Applied value		UUT Reading, dB	IEC 61672 Class 1 Specification, dB	
Range, dB	Freq. Weighting	Time Weighting	Level, dB	Frequency, Hz			
30-130	dBA	SPL	Fast	94	31.5	54.7	-39.4±2.0
					63	67.9	-26.2±1.5
					125	78.0	-16.1±1.5
					250	85.4	-8.6±1.4
					500	90.9	-3.2±1.4
					1000	94.1	Ref
					2000	95.5	+1.2±1.6
					4000	95.9	+1.0±1.6
				8000	92.5	-1.1+2.1; -3.1	

C-weighting

Setting of Unit-under-test (UUT)			Applied value		UUT Reading, dB	IEC 61672 Class 1 Specification, dB	
Range, dB	Freq. Weighting	Time Weighting	Level, dB	Frequency, Hz			
30-130	dBC	SPL	Fast	94	31.5	91.0	-3.0±2.0
					63	93.2	-0.8±1.5
					125	93.9	-0.2±1.5
					250	94.0	-0.0±1.4
					500	94.1	-0.0±1.4
					1000	94.1	Ref
					2000	94.1	-0.2±1.6
					4000	94.1	-0.8±1.6
				8000	90.6	-3.0 +2.1; -3.1	

5. Calibration Results Applied

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 61672 Class 1.

Uncertainties of Applied Value:

94 dB	31.5 Hz	± 0.05
	63 Hz	± 0.05
	125 Hz	± 0.05
	250 Hz	± 0.05
	500 Hz	± 0.05
	1000 Hz	± 0.05
	2000 Hz	± 0.05
	4000 Hz	± 0.05
	8000 Hz	± 0.10
104 dB	1000 Hz	± 0.05
114 dB	1000 Hz	± 0.05

The uncertainties are evaluated for a 95% confidence level.

Note:

The values given in this certification only related to the values measured at the time of the calibration and any uncertainties quoted will not allow for the equipment long-term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the calibration. (A+A)*L shall not be liable for any loss or damage resulting from the use of the equipment.

Certificate No.: APJ21-161-CC001



Page 4 of 4



CALIBRATION CERTIFICATE

Product : SOUND CALIBRATOR
Type : NC-75
Serial number : 34724243
Manufacturer : RION CO., LTD.
Calibration quantities : Sound pressure level (with reference standard microphone)
Calibration method : Measured by specified secondary standard microphone
according to JCSS calibration procedure specified by RION.
Ambient conditions : Temperature 23.9 °C, Relative humidity 49 %,
Static pressure 99.9 kPa
Calibration date : 05/07/2022 (DD/MM/YYYY)
Calibration location : 3-20-41 Higashimotomachi, Kokubunji, Tokyo 185-8533, Japan
RION CO., LTD. Calibration Room

We hereby certify that the results of this calibration were as follows.

Issue date : 11/07/2022 (DD/MM/YYYY)

Junichi Kawamura
Manager
Quality Assurance Section,
Quality Assurance Department,
Environmental Instrument Division,
RION CO., LTD.
3-20-41 Higashimotomachi, Kokubunji,
Tokyo 185-8533, Japan



This certificate is based on article 144 of the Measurement Law and indicates the result of calibration in accordance with measurement standards traceable to Primary Measurement Standards (National Standards) which realizes the physical units of measurement according to the International System of Units (SI).

The accreditation symbol is attestation of which the result of calibration is traceable to Primary Measurement Standards (National Standards).

The certificate shall not be reproduced except in full, without the written approval of the issuing laboratory.

The calibration laboratory who issued this calibration certificate conforms to ISO/IEC 17025:2017.

This calibration certificate was issued by the calibration laboratory accredited by IAJapan who is a signatory to the Mutual Recognition Arrangement (MRA) of International Laboratory Accreditation Cooperation (ILAC) and Asia Pacific Accreditation Cooperation (APAC). This (These) calibration result(s) may be accepted internationally through ILAC/APAC MRA.

CALIBRATION RESULT

1. Sound pressure level (with reference standard microphone)

Measured value	Expanded uncertainty *1
93.99 dB	0.09 dB

Specified secondary standard microphone:

Type : 4160
 Serial number : 2973341
 Reference Sound pressure : 2×10^{-5} Pa

*1 Defines an interval estimated to have a level of confidence of approximately 95 %.

Coverage factor $k=2$

Calibration result is the calibration value in ambient conditions during calibration.

BE OUT OF JCSS CALIBRATION

1. Frequency

Measured value	Measurement uncertainty ($k=2$)
1000.0 Hz	3.9×10^{-4} Hz

Working measurement standard universal counter:

Type : 53132A
 Serial number : MY40005574
 (JCSS Calibration Certificate No. 21081499079575510)

2. Total distortion

Measured value
0.2 %

Working measurement standard distortion meter:

Type : VA-2230A
 Serial number : 11076061
 (A2LA Calibration Certificate No. 1501-03080)

- closing -



輝創工程有限公司

Sun Creation Engineering Limited

Calibration & Testing Laboratory

Certificate of Calibration

校正證書

Certificate No. : C216243
證書編號

ITEM TESTED / 送檢項目 (Job No. / 序引編號 : IC21-2101) Date of Receipt / 收件日期 : 12 October 2021

Description / 儀器名稱 : Mini Anemometer
Manufacturer / 製造商 : RS PRO
Model No. / 型號 : RS-90
Serial No. / 編號 : 210722168
Supplied By / 委託者 : Acuity Sustainability Consulting Limited
Room C 11/F, Ford Glory Plaza, No. 37-39 Wing Hong Street,
Cheung Sha Wan, Kowloon

TEST CONDITIONS / 測試條件

Temperature / 溫度 : $(23 \pm 2)^{\circ}\text{C}$ Relative Humidity / 相對濕度 : $(50 \pm 25)\%$
Line Voltage / 電壓 : ---

TEST SPECIFICATIONS / 測試規範

Calibration check

DATE OF TEST / 測試日期 : 25 October 2021

TEST RESULTS / 測試結果

The results apply to the particular unit-under-test only.
The results are detailed in the subsequent page(s).

The test equipment used for calibration are traceable to National Standards via :

- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory
- Agilent Technologies / Keysight Technologies
- Testo Industrial Services GmbH, Germany
- Rohde & Schwarz Laboratory, Germany
- Fluke Everett Service Center, USA

Tested By : CKLo
測試 : C K Lo
Assistant Engineer

Certified By : H C Chan
核證 : H C Chan
Engineer

Date of Issue : 26 October 2021
簽發日期

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.

本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗所書面批准。

Sun Creation Engineering Limited – Calibration & Testing Laboratory
c/o 4/F, 1 Hing On Lane, Tuen Mun, New Territories, Hong Kong

輝創工程有限公司 - 校正及檢測實驗室

c/o 香港新界屯門興安里一號四樓

Tel/電話: (852) 2927 2606

Fax/傳真: (852) 2744 8986

E-mail/電郵: callab@suncreation.com

Website/網址: www.suncreation.com

Certificate of Calibration

校正證書

Certificate No. : C216243
證書編號

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 12 hours before the commencement of the test.
- Test equipment :

Equipment ID	Description	Certificate No.
CL018	Portable Calibrator	C204749
CL041 & CL041B	Digital Thermometer	C212654
CL042 & CL042B	Digital Thermometer	C212655
CL292	Recorder	C214057
CL330	Environmental Chamber	C205909
CL386	Multi-function Measuring Instrument	S16494

- Test procedure : MA006 & MA130N.

- Results :

4.1 Air Velocity

Applied Value (m/s)	UUT Reading (m/s)	Measured Correction		
		Value (m/s)	Measurement Uncertainty	
			Expanded Uncertainty (m/s)	Coverage Factor
2.01	1.70	+0.31	0.15	2.0
4.00	3.75	+0.25	0.20	2.0
6.01	5.81	+0.20	0.25	2.0
8.00	7.74	+0.26	0.29	2.0
10.01	9.84	+0.17	0.34	2.0

The results presented are the mean of 10 measurements at each calibration point.

4.2 Temperature

Applied Value (°C)	UUT Reading (°C)	Measured Correction		
		Value (°C)	Measurement Uncertainty	
			Expanded Uncertainty (°C)	Coverage Factor
25.0	24.8	+0.2	0.5	2.0

The results presented are the mean of 3 measurements at each calibration point.

Remarks : - The Measured Corrections are defined as :
Value = Applied Value - UUT Reading

- The expanded uncertainties are for a level of confidence of 95 %.

Note :


Only the original copy or the laboratory's certified true copy is valid.

The values given in this Certificate only relate to the values measured at the time of the test and any uncertainties quoted will not include allowance for the equipment long term drift, variations with environment changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the measurement. Sun Creation Engineering Limited shall not be liable for any loss or damage resulting from the use of the equipment.

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.

本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗室書面批准。

Water Quality



專業化驗有限公司
QUALITY PRO TEST-CONSULT LIMITED

Unit 10, 5/F, Wah Wai Centre, 38-40 Au Pui Wan St., Fotan, Hong Kong
Email: info@qualityprotest.com; Website: www.qualityprotest.com
Tel: (852) 3956 8717; Fax: (852) 3956 3928

REPORT OF EQUIPMENT PERFORMANCE CHECK/ CALIBRATION

Test Report No. : R-BC010056
Date of Issue : 18 January 2023
Page No. : 1 of 2

PART A - CUSTOMER INFORMATION

Acuity Sustainability Consulting Limited
Unit E, 12/F, Ford Glory Plaza 37-39 Wing Hong Street, Cheung Sha Wan, Kowloon, Hong Kong

PART B - SAMPLE INFORMATION

Name of Equipment : HORIBA U-53
Manufacturer : HORIBA
Serial Number : PORBNFNT
Date of Received : 12 January 2023
Date of Calibration : 17 January 2023
Date of Next Calibration : 16 April 2023
Request No. : D-BC010056

PART C - REFERENCE METHODS/ DOCUMENTS FOR THE CALIBRATION

Test Parameter	Reference Method
pH value	APHA 21e 4500 H ⁺
Temperature	Section 6 of international Accreditation New Zealand Technical Guide no. 3 Second edition March 2008: Working Thermometer Calibration Procedure
Salinity	APHA 21e 2520 B
Dissolved oxygen	APHA 21e 4500 O
Turbidity	APHA 21e 2130 B

PART D - CALIBRATION RESULT

(1) pH value

Target (pH unit)	Display Reading (pH unit)	Tolerance	Result
4.00	3.94	-0.06	Satisfactory
7.42	7.54	0.12	Satisfactory
10.01	9.92	-0.09	Satisfactory

Tolerance of pH value should be less than ± 0.2 (pH unit)

(2) Temperature

Reading of Ref. thermometer (°C)	Display Reading (°C)	Tolerance	Result
10	11.03	1.03	Satisfactory
23	24.48	1.48	Satisfactory
33	34.19	1.19	Satisfactory

Tolerance of Temperature should be less than ± 2.0 (°C)

(3) Salinity

Expected Reading (g/L)	Display Reading (g/L)	Tolerance (%)	Result
10	9.51	-4.90	Satisfactory
20	19.04	-4.80	Satisfactory
30	29.62	-1.27	Satisfactory


Tolerance of Salinity should be less than ± 10.0 (%)

--- CONTINUED ON NEXT PAGE ---

AUTHORIZED
SIGNATORY:

LEE Chun-ning

Assistant Manager (Chemical Testing)



專業化驗有限公司
QUALITY PRO TEST-CONSULT LIMITED

Unit 10, 5/F, Wah Wai Centre, 38-40 Au Pui Wan St., Fotan, Hong Kong
Email: info@qualityprotest.com; Website: www.qualityprotest.com
Tel: (852) 3956 8717; Fax: (852) 3956 3928

REPORT OF EQUIPMENT PERFORMANCE CHECK/ CALIBRATION

Test Report No. : R-BC010056
Date of Issue : 18 January 2023
Page No. : 2 of 2

(4) Dissolved oxygen

Expected Reading (mg/L)	Display Reading (mg/L)	Tolerance	Result
9.00	8.78	-0.22	Satisfactory
5.88	5.44	-0.44	Satisfactory
2.65	2.25	-0.40	Satisfactory
1.14	0.80	-0.34	Satisfactory

Tolerance of Dissolved oxygen should be less than ± 0.5 (mg/L)

(5) Turbidity

Expected Reading (NTU)	Display Reading (NTU)	Tolerance (%)	Result
0	0.11	--	Satisfactory
10	10.0	0.0	Satisfactory
20	21.5	7.3	Satisfactory
100	108	8.0	Satisfactory
800	812	1.5	Satisfactory

Tolerance of Turbidity should be less than ± 10.0 (%)

Remark(s)

- The "Date of Next Calibration" is recommended according to best practice principals as practiced by QPT or quoted form relevant international standards.
- The results relate only to the calibrated equipment as received
- The performance of the equipment stated in this report is checked with independent reference material and results compared against a calibrated secondary source.
- "Displayed Reading" denotes the figure shown on item under calibration/ checking regardless of equipment precision or significant figures.
- The "Tolerance Limit" mentioned is the acceptance criteria applicable for similar equipment used by Quality Pro Test-Consult Ltd. or quoted form relevant international standards.

--- END OF REPORT ---



Calibration Certificate

Certificate No. **210252**

Page 1 of 2 Pages

Customer : Acuity Sustainability Consulting Limited

Address : Unit E, 12/F, Ford Glory Plaza, No. 37-39 Wing Hong Street, Cheung Sha Wan, Kowloon, H.K.

Order No. : Q24081

Date of receipt : 31-Oct-22

Item Tested

Description : Flow Probe

Manufacturer : Global Water

Model : FP111

I.D. : --

Serial No. : 22K100859

Test Conditions

Date of Test : 7-Nov-22

Ambient Temperature : 23°C

Supply Voltage : --

Relative Humidity : 78%

Test Specifications

Calibration check.

Ref. Document/Procedure : V12

Test Results

All results were within the manufacturer's specification.

The results are shown in the attached page(s).

Main Test equipment used:

<u>Equipment No.</u>	<u>Description</u>	<u>Cert. No.</u>	<u>Traceable to</u>
S179	Std. Tape	201868	NIM-PRC
S136A	Stop Watch	201878	SCL-HKSAR

The values given in this Calibration Certificate only relate to the values measured at the time of the test and any uncertainties quoted will not include allowance for the equipment long term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the measurement. Hong Kong Calibration Ltd. shall not be liable for any loss or damage resulting from the use of the equipment.

The test equipment used for calibration are traceable to International System of Units (SI), or by reference to a natural constant.
The test results apply to the above Unit-Under-Test only

Calibrated by : 
Kin Wong

Approved by : 
Alan Chu

This Certificate is issued by:
Hong Kong Calibration Ltd.

Unit 8B, 24/F., Well Fung Industrial Centre, No. 58-76, Ta Chuen Ping Street, Kwai Chung, NT, Hong Kong.
Tel: 2425 8801 Fax: 2425 8646

Date: 7-Nov-22



Calibration Certificate

Certificate No. 210252

Page 2 of 2 Pages

Results :

Applied Value (m/s)	UUT Reading (m/s)	Mfr's Spec.
0.96	1.0	± 0.1 m/s

Remarks : 1. UUT : Unit-Under-Test

2. Uncertainty : ± 1 %, for a confidence probability of not less than 95%.

----- END -----